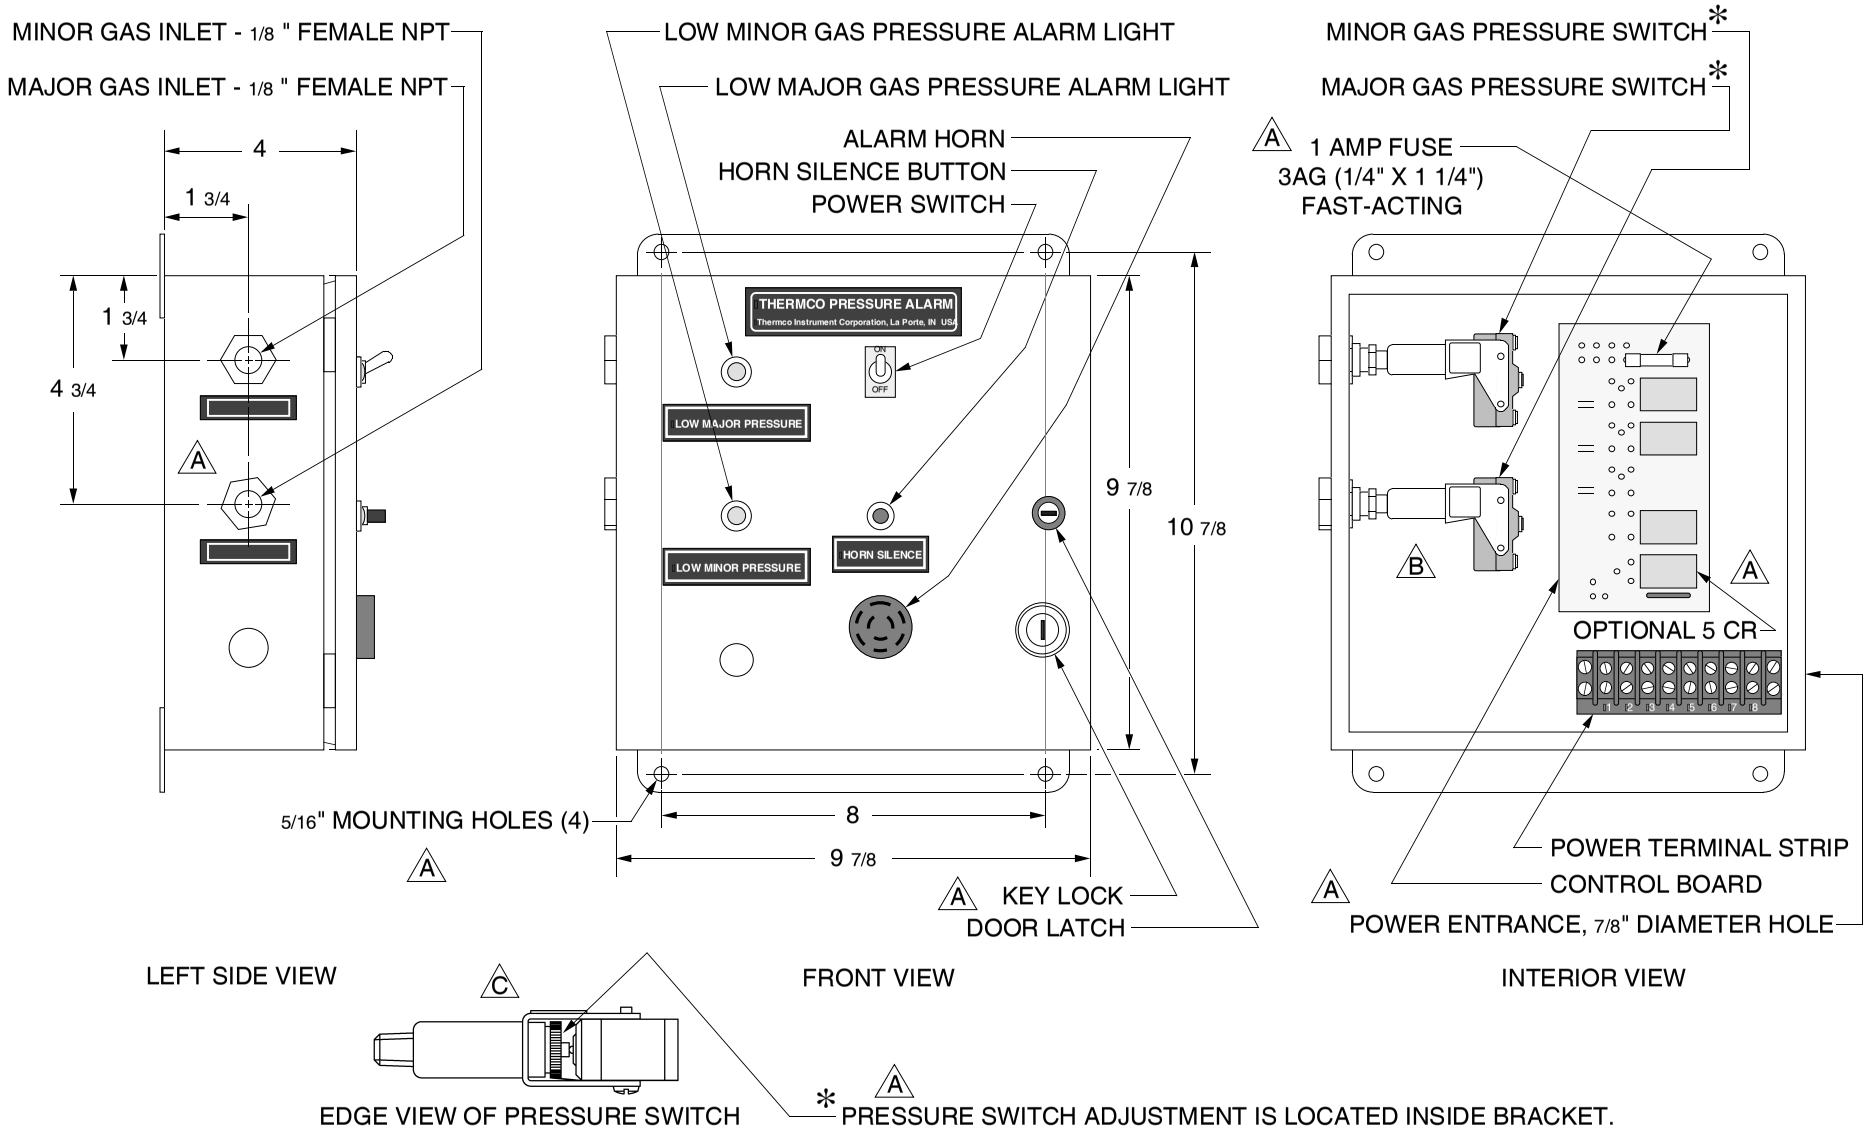

F			
E			
D			
C	CORRECTED INFORMATION ABOUT PRESSURE SWITCH ADJUSTMENT; ADDED VIEW	GAR	2-26-08
B	REPLACED INLET PRESSURE SWITCHES WITH U.E. J40 SWITCHES	KGR	3-12-07
A	ADDED INLET LABELS; ADDED MOUNTING HOLE INFO; ADDED PRESSURE SWITCH ADJUSTMENT INFO; ADDED POWER ENTRANCE INFO; ADDED KEY LOCK AND DOOR LATCH INFO; ADDED FUSE INFO; ADDED 5 CR INFO; MOVED RELAY BOARD; ADDED "115 VAC" TO DRAWING TITLE	GAR	12-10-02
	REVISIONS	BY	DATE

THERMCO INSTRUMENT CORPORATION
LA PORTE, INDIANA USA

SCALE: N.T.S.	B. M. NO:	S. O. NO:	DRAWN BY: DB
DATE: 8-15-02	CUSTOMER:		APPROVED BY:
TITLE: INSTRUCTION DRAWING FOR MODEL 9502 PRESSURE ALARM SYSTEM, 115 VAC (A)			SUPERSEDES:
			DRAWING NUMBER: 1-12108