




**NOTE:**  
GAS ANALYZER REQUIRES 14 INCHES OF CLEARANCE FOR DOOR SWING.

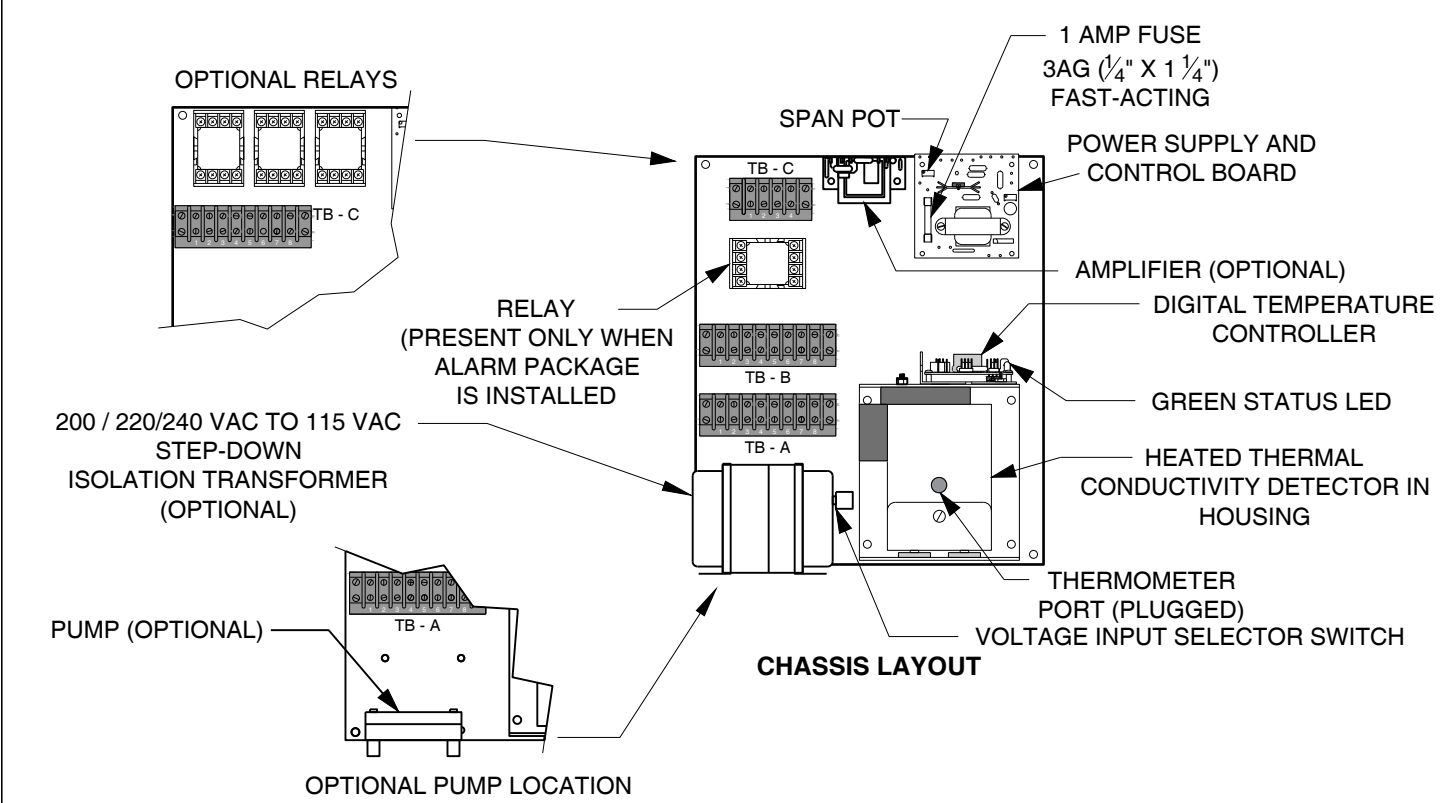

STEP-DOWN TRANSFORMER VOLTAGE INPUT SELECTOR SWITCH SETTINGS	
DO NOT ADJUST THIS SETTING UNLESS YOU HAVE CONSULTED WITH THE FACTORY	
NOMINAL AC INPUT VOLTAGE	INPUT SELECTOR SWITCH SETTING
200	210
220	230
240	250

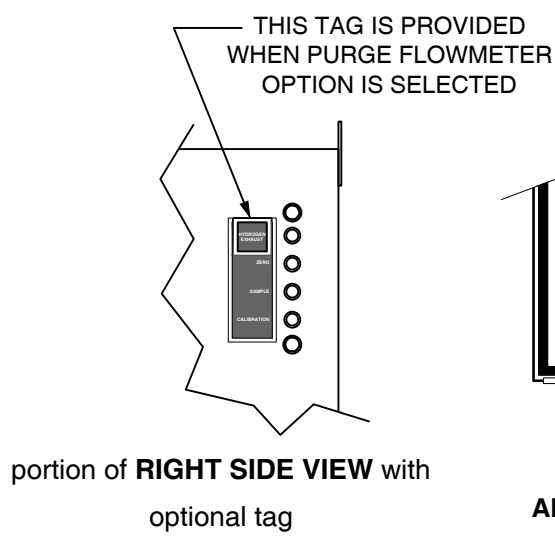

- NOTES:**
- ALL DIMENSIONS ARE IN INCHES UNLESS OTHERWISE INDICATED.
  - REFER TO DATA SHEET TO DETERMINE WHICH OPTIONS ARE PRESENT.

H G F E D C B A			 INSTRUMENT CORPORATION LA PORTE, INDIANA USA	DATE: 9-9-20
				SCALE: N.T.S.
				DRAWN BY: JTM
				APPROVED BY: <i>Gar</i>
	GRAPHICAL UPDATES; ADDED SAMPLE PORT NOTE	GAR	9-3-20	SUPERSEDES: 2-13244
	REVISIONS	BY	DATE	DRAWING NUMBER: 2-14591

TITLE: INSTRUCTION DRAWING FOR MODEL 7010 GAS ANALYZER